

Product datasheet

Note: This protocol was modified as of December 2017. All previous protocols are obsolete.

Human CRP ELISA Kit

Product #: 0040

Storage recommendations

Store the kit at 2-8°C. The kit is stable for a period of up to 4 months from the date of receipt.

Description

This human CRP ELISA kit is designed to enable the quantitative measurement of natural and/or recombinant CRP in serum, plasma and cell culture media only. The kit contains one strip-well plate pre-coated with human CRP capture antibody along with sufficient key reagents for plate development.

Reagent preparation

Wash buffer (20x) and Assay diluent 3BT (2x)

If crystals have formed in the concentrate, warm to room temperature and mix well. Once all the visible crystals have dissolved, for wash buffer, dilute 25mL of wash buffer concentrate in 475mL of distilled water to make 500mL of wash buffer; for 3BT, dilute 25mL of 3BT (2x) in 25mL of distilled water to make 50mL of 3BT.

Standard

The standard is present in lyophilised form with the amount of standard present in the tube clearly stated on the label. Prior to reconstitution, briefly centrifuge the vial to ensure that any loose lyophilised material has collected at the bottom of the tube.

For cell culture samples:

Reconstitute the standard in 1mL of assay diluent 3BT and mix well by inversion. **Allow the standard to dissolve for at least 15 minutes with regular inversion prior to use.** Dividing the amount of lyophilised standard (as per the label) by 1mL will give the standard concentration. **Use sample culture medium to perform the serial dilutions.**

For serum and plasma samples:

Reconstitute the standard in 1ml of assay diluent 3BT and mix well by inversion. **Allow the standard to dissolve for at least 15 minutes with regular inversion prior to use.** Dividing the amount of

lyophilised standard (as per the label) by 1mL will give the standard concentration. **Use assay diluent 3BT to perform the serial dilutions.**

The standard curve should be performed in duplicate starting at 50ng/mL and diluted 1 in 2 down to at least 0.78ng/mL. Use the formula $C_1V_1=C_2V_2$ to calculate the amount of stock required to make 1mL of the 50ng/mL standard. Perform this initial dilution in a micro tube ensuring that the appropriate diluent is used. Serial dilutions are then easily achieved by using a micro-titre plate (or similar). Load 300µL of the 50ng/mL standard into the first 2 wells of the dilution plate and load 125µL of the appropriate diluent into the remaining wells. Using a multichannel pipette, transfer 125µL from the first wells (i.e. 50ng/mL) into the second wells (now 25ng/mL), mix well by pipetting up and down before transferring 125µL to the next wells (now 12.5ng/mL). Repeat until the serial dilution is complete.

Sample preparation.

Serum or Plasma should be diluted 1 in 1000 prior to assay. A suggested 1 in 1000 dilution is 5µL of serum into 495µL of assay diluent 3BT for 100 fold dilution. Then 10µL of diluted serum or plasma is added into 90µL of 3BT to make final 1000 dilution.

Detection antibody

Briefly centrifuge prior to use. The anti-human CRP Biotin labelled detection antibody is provided in a liquid form at the concentration specified on the tube. **The anti-human CRP-Biotin labelled detection antibody should be diluted to 50ng/ml in assay diluent 3BT immediately prior to use.**

Streptavidin-HRP conjugate

Briefly centrifuge prior to use. The streptavidin-HRP conjugate should be diluted 500 fold in assay diluent 3BT immediately prior to use. For example, if developing the entire plate aliquot 22µL of streptavidin-HRP conjugate into 11mL of assay diluent 3BT.

Protocol

It is highly recommended that all standards, samples and zero standard controls be performed in duplicate. Ensure that all reagents are at room temp prior to use.

1. Prepare solutions as required by following the instructions outlined in the reagent preparation section.
2. Remove any 8 well strips that are not required for the assay and place back in the foil pouch ensuring that it is closed tightly.

3. Add 50 µL of assay diluent 3BT to each well.
4. Add 50µL of standards, samples* (**Serum/Plasma samples require dilution. Refer to sample preparation section**) and zero standard controls to each well and seal the plate with the adhesive cover provided. Incubate for 2 hours at room temperature.
5. Aspirate each well and wash the plate 4x with wash buffer (250µL). Washing can be achieved with a multichannel pipette, plate washer or similar. To remove residual wash buffer invert the plate and tap the plate on paper towels between each wash.
6. Add 100µL of biotin labelled detection antibody to each well and seal the plate with the adhesive cover provided. Incubate for 1 hour at room temperature.
7. Repeat the aspiration/wash steps in step 5.
8. Add 100µL of freshly diluted streptavidin-HRP conjugate to each well and seal the plate with the adhesive cover provided. Incubate for 45 minutes at room temperature.
9. Aspirate each well and wash the plate **5x** with wash buffer (250µL) as per step 4. It is important to wash thoroughly here to reduce unwanted background.
10. Add 100µL of TMB substrate to each well and incubate for approximately 15 minutes at room temperature. **Ensure the plate is protected from light.** Check the development process (blue colour) every 5 minutes or so to prevent over development of the plate.
11. Stop the reaction with 50µL of stop solution. The wells will turn from blue to yellow in colour.
12. Determine the optical density (OD) of the plate using a micro-plate reader set at 450nm. If the micro-plate reader allows wavelength correction, set at 570nm.

Calculation of results


Calculate the mean absorbance for each standard, sample and control and subtract the mean of the zero standard controls.

Create a standard curve by plotting the mean OD of each standard on the y-axis versus the standard concentration on the x-axis. If available, use a program capable of generating a four parameter logistic (4-PL) curve fit. A free user friendly 4-PL program is available online at <http://elisaanalysis.com>. Alternatively, plot a best fit curve through the standard points and overlay a linear or polynomial trend-line. The resultant equation displayed on the graph can then be used to calculate the unknown concentrations by solving for x. When fitting a trend-line it is essential that the r^2 value is 0.99 or higher. If not, then simply find the linear portion of the graph by removing the higher standard points from the analysis.

If the samples were diluted then multiply the concentration read from the standard curve by the dilution factor.

Standard curve

This is a representative example of a typical standard curve. A separate standard curve must be generated for each experiment.

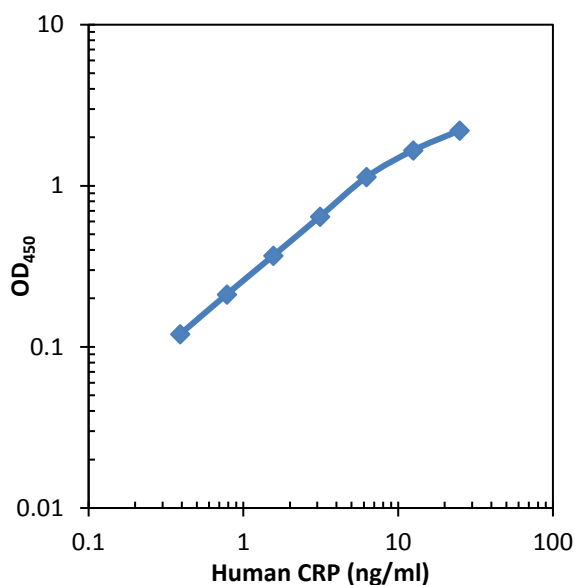

Sensitivity

The lower limit of quantitation (LLQ) of the assay is typically <0.1ng/ml.

The LLQ was determined by adding 3 standard deviations to the mean optical density of 5 zero antigen replicates and calculating the corresponding concentration.

Precision.

Intra-assay CV: <10%

Inter-assay CV: <10%

Recovery.

Pooled human sera (1:100) was spiked with recombinant human CRP and compared to a spiked assay diluent control. Typical values are as follows.

Control values (ng/ml)	Serum values (ng/ml)	Recovery (%)
12.28	9.95	81
6.55	5.68	86
3.35	2.7	81

Linearity.

Linearity of dilution was determined by serially diluting spiked samples and analysing them in the ELISA. Serum values were corrected for endogenous levels of CRP.

Sample	Dilution factor	Expected (ng/ml)	Observed (ng/ml)	Recovery (%)
Serum	1:1000	9.95	-	-
	1:2000	4.97	5.68	114
	1:4000	2.48	2.7	108

Cross reactivity

This ELISA kit recognises natural and recombinant human CRP. No significant cross-reaction with human IL-8, IL-1 β or MCP-3.

Technical hints

Always ensure complete reconstitution and/or dilution of reagents prior to use.

To ensure uniform temperature/humidity levels for all steps of the ELISA across the entire plate it is often beneficial to perform the incubations in a humidity chamber. This can simply be a Styrofoam box containing moistened paper hand towels.

Plates should always be incubated with the adhesive plate sealer in place.

Always ensure accurate pipetting of reagents at all times, especially the standards.